

Freestanding Track Specifications




Specifications:

The free-standing track is a load bearing portable track set up that can be moved around from room to room as required. The free-standing track is designed to be used with either the GoLift 400 or the GoLift Portable 450. The stand comes as five separate pieces that require three different Allen keys in order to set up.

- Maximum Capacity: 450lbs
- Set up time: 5 minutes
- Compatible with any Amico trolley
- 4-point contact design for auto leveling on uneven flooring
- Handset charging compatible, optional wall mounted dock charging station separately available
- Does not come with charger.
- No maintenance or servicing required

WARNING: the stand must be used on level ground (don not use at an angle). The lift must only be operated while the patient is on the inside of the outer frame of the stand on wither side.


Dimensions:

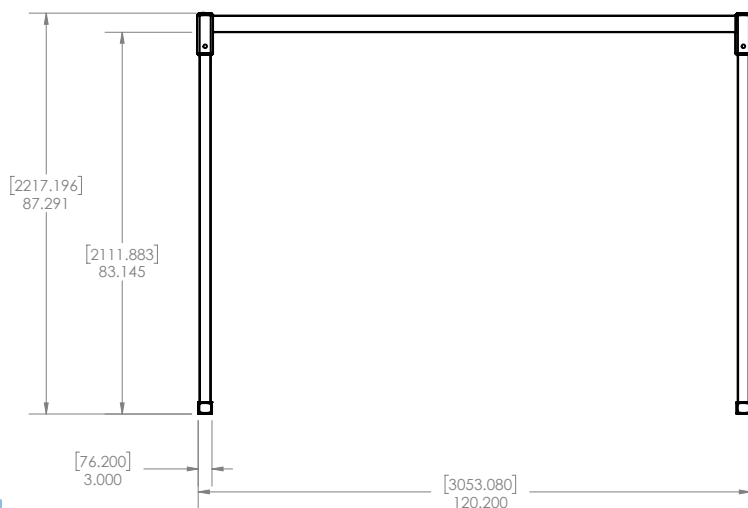

Part Numbers:

- 87" Height, 120" Length: TRK-PORT-80-120-ASSY
- 99" Height, 120" Length: TRK-PORT-92-120-ASSY
- 87" Height, 135" Length: TRK-PORT-80-135-ASSY
- 99" Height, 135" Length: TRK-PORT-92-135-ASSY
- 87" Height, 149" Length: TRK-PORT-80-149-ASSY
- 99" Height, 149" Length: TRK-PORT-92-149-ASSY

NOTE: Must follow maximum span chart: 135" for 450 lbs & 149" for 400 lbs (custom length available upon request):

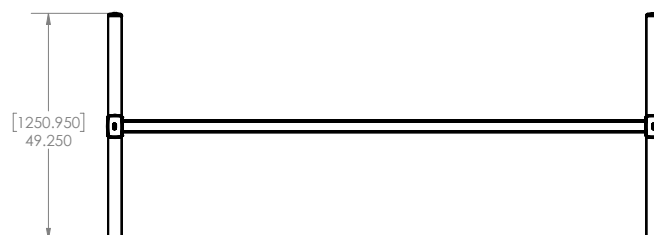


How to Assemble

Recommended: Two (2) People

Tools: 5/16" Allen Key, 7/32" Allen Key

Step 1:


Line up the holes in the foot with the threaded holes on post and use the 3/6-18 x 1" long socket cap screws to secure the foot to the posts.

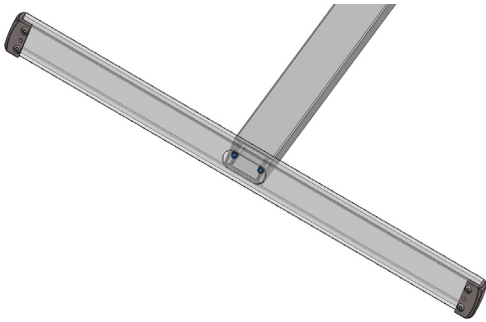

Step 2:

Stand the two posts up and drop the track assembly (shown in blue) onto the two posts.

Note: The tracks must be straight, the fit is tight.

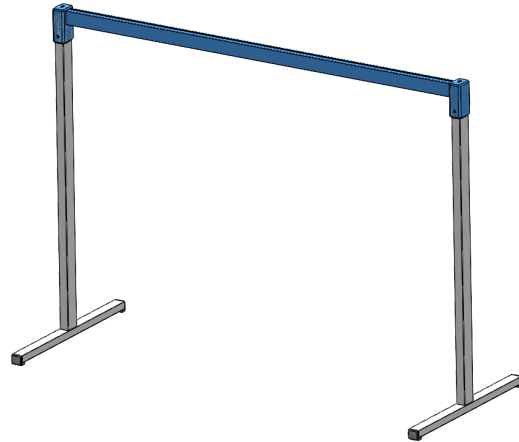

Step 3:

Align the mounting holes in the post and the track assembly and use the 3/8" socket cap screws on either side to secure the track assembly to the posts. Press the caps over the screws to hide them from view.

